




# Mobel Biomaterials Technology Co.,ltd

Add: 25 No.Bio-chemicals Technical Zoon,Yuhang District, Hangzhou city,Zhejiang P.R China 310000

www.mobelbiochem.com Email: sales@mobelbiochem.com Tel: +86-571-85099223 Fax:+86-571-85099222

602694

## MASS SPECTROMETRY REPORT

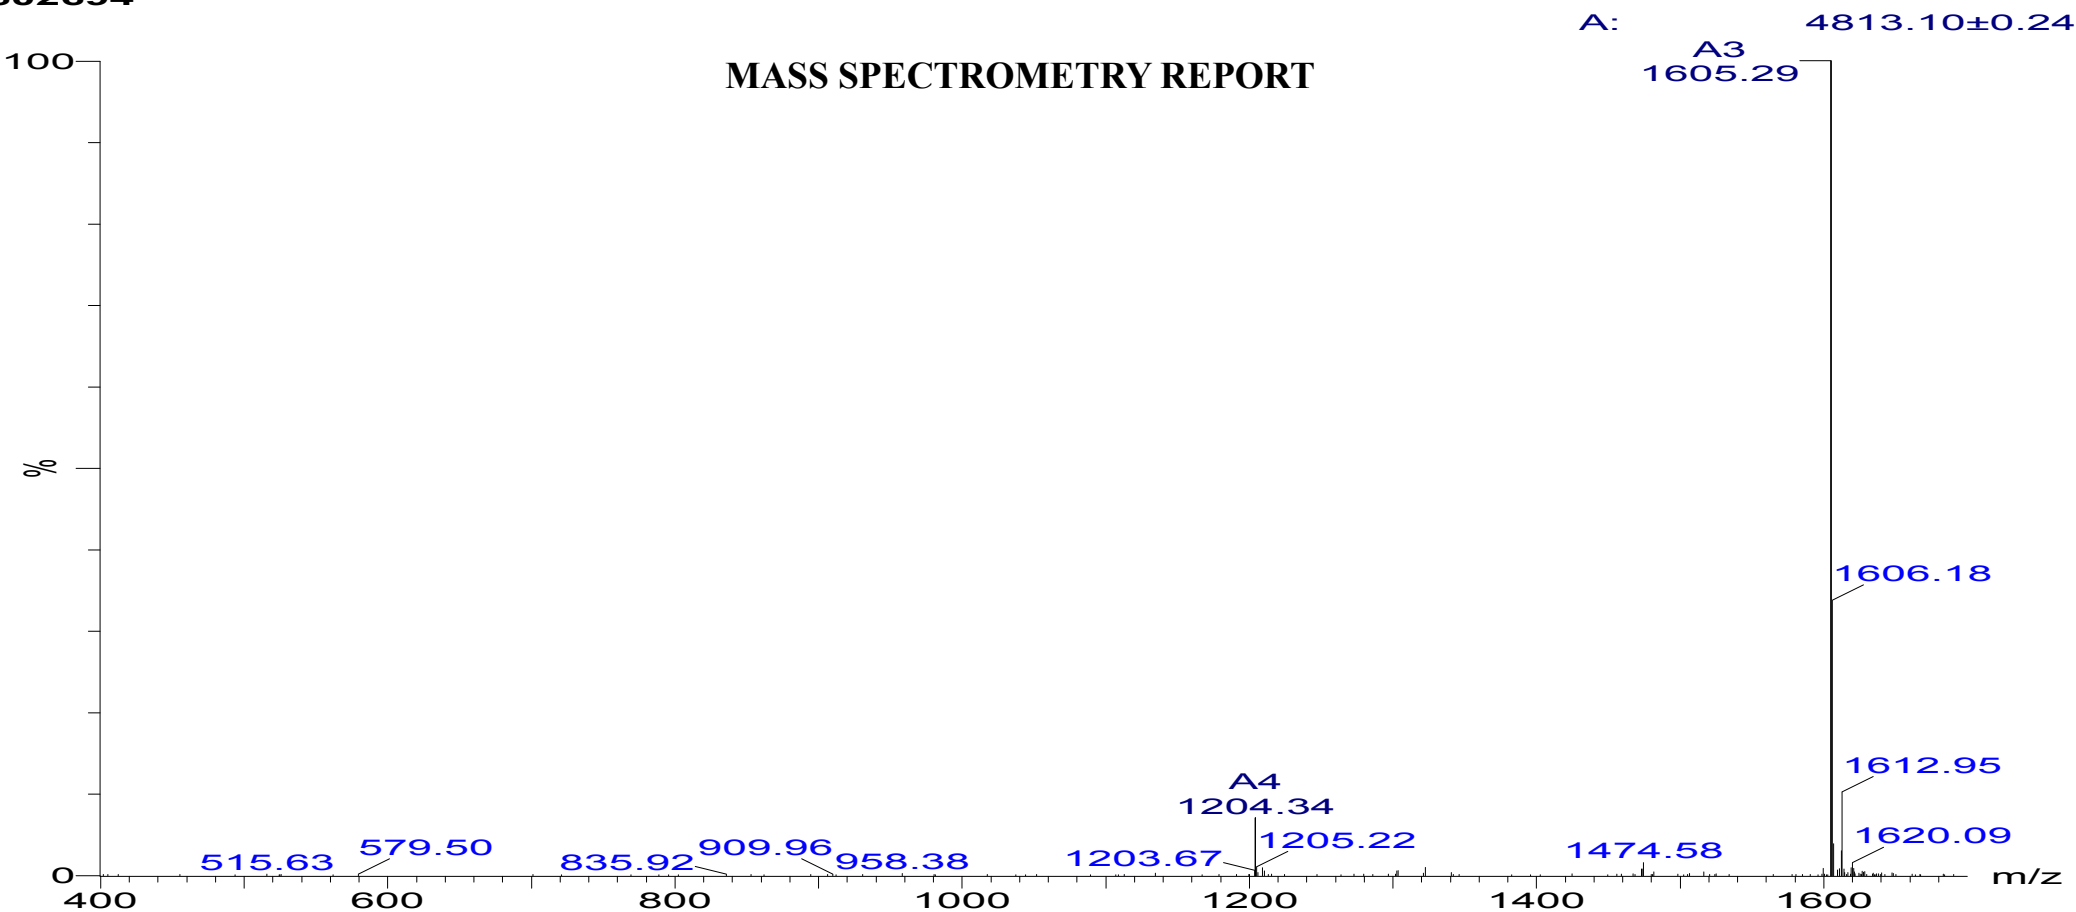

### Sample Description

Analyzed date: 2023-07-20  
Analyst: SHAO  
Sample: 602694  
M.W.: 4813.5  
Lot. No.:

### Instrument

Waters 2695  
Probe: ESI  
Nebulizer Gas Flow: 1.5L/min  
CDL: -20.0v  
CDL Temp.: 250 °C  
Block Temp.: 200 °C

Probe Bias: +4.5kv  
Detector: 1.5kv  
T. Flow: 0.5ml/min  
B. Conc.: 50%H2O/50%ACN